

Surgical Technique For Periarticular Distal Radial Locking Plates

This surgical technique developed
in conjunction with:

Douglas P. Hanel, M.D.

Professor, Department of
Orthopaedics and Sports Medicine
University of Washington
Seattle, Washington

Thomas F. Varecka, M.D.

Professor of Orthopaedic Surgery
University of Minnesota Medical School
Faculty, Hennepin County
Medical Center
Minneapolis, Minnesota

Table of Contents

Introduction

Locking Screw Technology	3
Locking Plate Technology	3
Plate Features	3
Indications	3
Fracture Classification	4
The Three-Column Theory of Distal Radius Fracture Fixation	4
Volar Fixation of Fractures of the Distal Radius	5
Treatment Algorithm	6

Surgical Technique

Preoperative Preparation	8
Fracture Reduction	8
Volar Approach	8
Dorsal Approach	9
Plate Positioning	10
Fracture Fixation	11
Implant Removal	12

Instruments and Implants

Ordering Information

Introduction

The *Zimmer* Periarticular Locking Plate System combines locking screw technology with periarticular plates to create fixed-angle constructs for use in multifragmentary fractures or where deficient bone stock or poor bone quality is encountered. The fixed-angle plate/screw device can be used in osteopenic bone and other areas where traditional screw fixation may be compromised.

The Periarticular Locking Plates will accommodate standard screws, as well as locking screws with threaded heads. When necessary, interfragmentary compression can be achieved with lag screws.

All plate configurations contain locking screw holes in the plate head and alternating locking and compression screw holes in the shaft. The locking screw holes will accept either conical or locking screws.

The distal radius plates will accept 2.4mm Locking Screws, 2.4mm Conical Screws and 1.8mm Locking Pegs in the plate head. The plate shaft will accept 2.4mm Conical Screws and 2.4mm Locking Screws in the threaded holes, 2.4mm Conical Screws and 2.7mm Cortical Screws in the first slot and 3.5mm Cortical Screws with 2.7mm head in the compression slots.

Locking Screw Technology

The heads of the locking screws contain male threads while the holes in the plates contain female threads. This allows the screw head to be threaded into the plate hole, locking the screw into the plate. This technical innovation provides the ability to create a fixed-angle construct while using familiar plating techniques.

Locking Plate Technology

By using locking screws in a bone plate, a fixed-angle construct is created. In osteopenic bone or fractures with multiple fragments, secure bone purchase with conventional screws may be compromised. Locking screws do not rely on bone/plate compression to resist patient load, but function similarly to multiple small angled blade plates. In these cases, the ability to lock screws into a fixed-angle construct is imperative.

By combining locking screw holes with compression screw holes in the shaft, the plate can be used as both a locking device and a fracture compression device. If compression is desired, it must be achieved first by inserting the standard screws in the compression screw holes before inserting any locking screws.

The locking plate design does not require compression between the plate and bone to accommodate loading. Therefore, screw thread purchase in the bone can be achieved with a thread depth less than that of traditional screws. The shallow thread profile, in turn, allows for screws with a larger core diameter to accommodate loading with improved bending and shear strength.

Plate Features

Features of the Periarticular Locking Plate include:


- Plates are precontoured to help with metaphyseal/diaphyseal reduction
- Thick-to-thin plate profiles make the plates autocontourable
- Anatomical contouring of the plates matches the shape of the distal radius
- Low plate profile facilitates fixation without impinging on soft tissue
- Plates are available in left and right configurations, in a variety of lengths

Indications

The Periarticular Locking Plate System

is indicated for temporary internal fixation and stabilization of osteotomies and fractures, including:

- Comminuted fractures
- Supracondylar fractures
- Intra-articular and extra-articular condylar fractures
- Fractures in osteopenic bone
- Nonunions
- Malunions

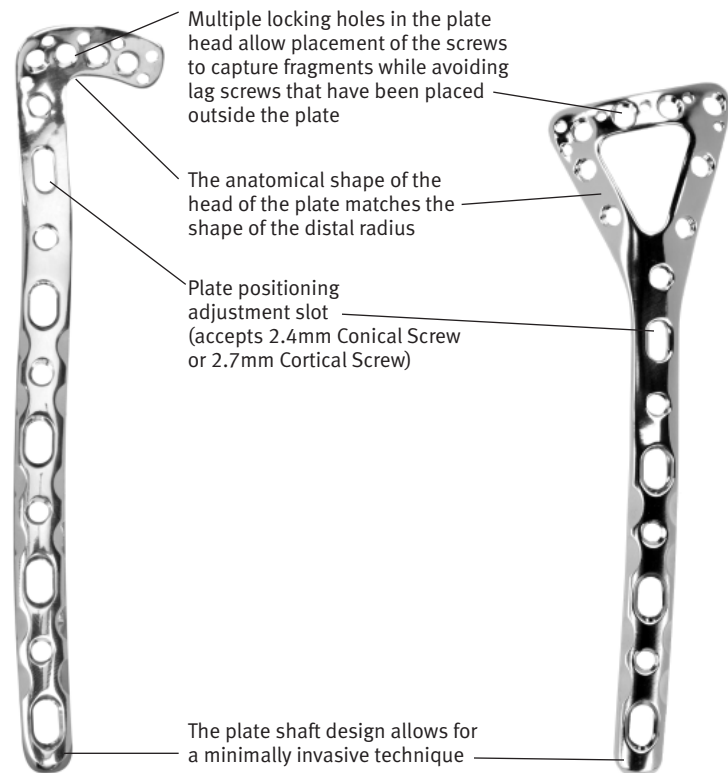

Volar Lateral Column Plate

Dorsal Delta Plate

Fracture Classification

The AO classification for long bone fractures is divided into three general groups, each with three subgroups. The groups are extra-articular, partial articular, and complex articular. The subgroups reflect the degree of metaphyseal comminution.

Refer to the **AO Comprehensive Classification of Fractures of Long Bones** for more specific information.

The Three-Column Theory of Distal Radius Fracture Fixation

The Three-Column theory of distal radius fracture fixation includes the following (Fig. 1):

- Lateral Column – The lateral side of the radius including the radial styloid and the scaphoid fossa
- Intermediate Column – The ulnar side of the radius, including the lunate fossa and the sigmoid notch
- Medial Column – The ulnar head, including the triangular fibrocartilage complex (TFCC) and the ulnar part of the distal radioulnar joint (DRUJ)



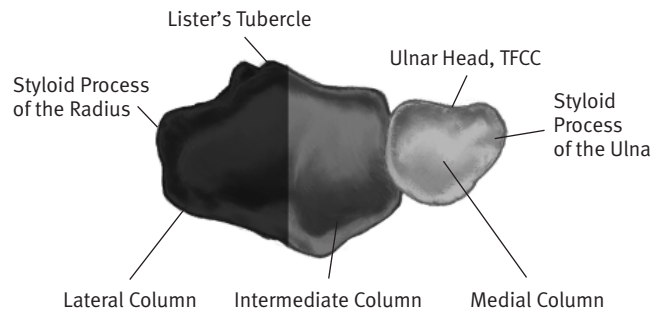


Fig. 1

Rikli DA, Regazzoni P. Fractures of the Distal End of the Radius Treated by Internal Fixation and Early Function. *J Bone Joint Surg.* 1996;78-B(4):588-9.

Volar Fixation of Fractures of the Distal Radius

A volar approach is typically used for volarly displaced fractures and may be utilized for some dorsally displaced fractures (Fig. 2).

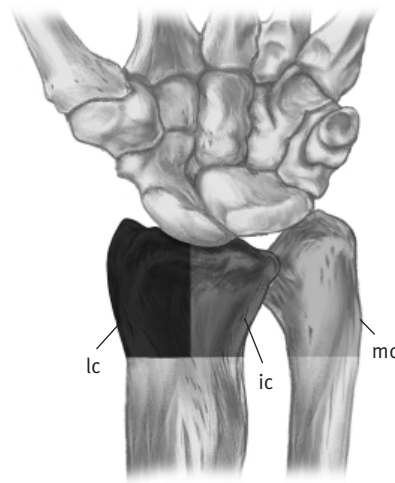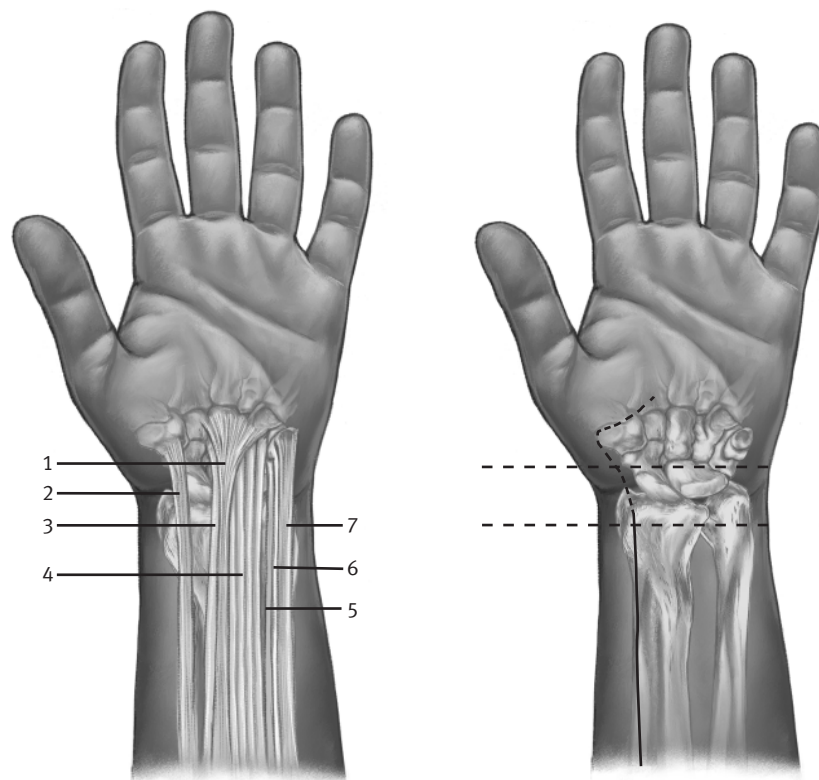

a) Surgical anatomy of palmar aspect

b) Skin incision

1) Palmaris longus muscle, 2) Flexor carpi radialis (FCR), 3) Median nerve, 4) Flexor digitorum profundus (FDP), 5) Ulnar artery, 6) Ulnar nerve, 7) Flexor carpi ulnaris (FCU)

Fig. 2

Treatment Algorithm

Fracture of the distal radius

Non-displaced

- Plaster cast or splint and/or percutaneous pinning
- Follow-up
 - Weekly x-rays. If reduction is lost then by definition the fix is unstable and should be treated with more than cast immobilization
- Secondary displacement or metaphyseal comminution (involving more than $\frac{1}{3}$ of the diaphysis on lateral projection)
 - Closed reduction and percutaneous pinning and/or external fixation (with or without bone graft)
 - Plate fixation
- After Care: See Postoperative Management

Displaced

Reducible

Extra-articular (AO ASIF Type A)

- Closed reduction then same as Non-Displaced Intra-articular (AO ASIF Types B and C)
- Closed reduction
 - Stable (infrequent)
 - Plaster cast or splint
 - After Care: See Postoperative Management
 - Secondary displacement
 - Closed reduction
 - Percutaneous pinning
 - Percutaneous pinning & external fixation (with or without limited open incisions and with or without bone graft)
 - Plate fixation (with or without bone graft)

After Care: See Postoperative Management

Irreducible/Unstable

Extra-articular

- Closed reduction and percutaneous pinning (assisted by image intensification)
- External fixation (with or without bone graft and percutaneous pinning)
- Plate fixation (with or without bone graft)

Intra-articular

- Limited open reduction, bone graft, percutaneous fixation and external fixation
- Open reduction plate fixation (volar vs dorsal, fixed angle vs conventional)

Postoperative Management

If treated by closed casting, then follow up radiographs are obtained weekly for a minimum of three weeks after injury. Radiographs are compared to the initial reduction.

If treatment is percutaneous or open, then the frequency of radiographs is predicated upon the surgeon's interpretation of fixation stability.

Initial immobilization is in a long arm splint with the wrist neutral and the forearm in supination.

Edema control and digit motion are started straight away.

Splint and cast are changed to short arm devices when the DRUJ is considered stable.

Patients often have difficulty regaining or maintaining forearm supination.

In those patients with stable DRUJ's, long arm splints with the forearm in supination and the wrist in slight extension are worn until supination is easily maintained.

External Fixators, when used, require daily pin tract care. Crusts are removed with soap and water, and the patient must keep the sites dry. Gauze or sponge bumpers are used to minimize motion about the skin pin interface.

Both radiocarpal motion and grip strength follow closely after regaining forearm and digit motion. Strengthening exercises and radiocarpal motion are not typically emphasized until after evidence of fracture healing and return of forearm and digit motion.

Surgical Technique

Preoperative Preparation

After assessing the fracture radiographically and preparing a preoperative plan, place the patient in the supine position with the hand and arm on a radiolucent hand table. Be sure that the fluoroscope can be positioned to visualize the distal radius in both the lateral and A/P views.

Fracture Reduction

It is imperative that accurate reduction of the joint be obtained prior to, and maintained during, application of the distal radius plate. The initial reduction is assisted by continuous finger trap traction in the standard horizontal upper extremity operating position and is visualized by intraoperative image intensification. Agee's reduction maneuver provides a survey of metaphyseal stability and articular incongruity. The maneuver assists in reduction, but continuous traction may interfere with the application of plates and screws, especially those implants placed volarly. To that end, provisional fixation and frequent assessment of reduction maintenance with image intensification will be required if traction is removed. Attempting to apply the radius plate without such traction risks fixing the fracture in an unreduced position and may make the sequencing of the procedure very difficult.

* Agee JM. Unstable fracture dislocations of the proximal interphalangeal joint. Treatment with the force couple splint. *Clin Orthop*. 214:101-112, 1987.

A closed reduction is performed in the following manner:*

1. Apply ten pounds of longitudinal traction to restore overall length. (It may even restore, but not maintain, intra-articular step off in fractures treated shortly after injury.)
2. Translate the hand and radiocarpal joints volarly relative to the forearm. This will restore palmar tilt and, more importantly, will reveal unstable volar shearing fractures such as those associated with the volar medial corner of the radius in severely comminuted fractures, or those associated with the more typical shearing fractures that are often referred to as Smith-Barton fractures.
3. Slightly pronate the hand and deviate ulnarly relative to the forearm (NOT Forearm pronation relative to the elbow). This restores radial inclination and the rotatory component of fractures that result from falls onto outstretched hands.

Volar Approach

Fractures that are volarly unstable require volar stabilization. These are the fractures that involve the volar aspect of the lateral and intermediate columns. The most obvious are shearing fractures referred to with the eponym Smith/Barton, or high energy compression fractures that split the sigmoid notch in a coronal plane.

In addition, one must be aware that a rather innocuous appearing fracture that involves the volar medial corner can result in volar radiocarpal fracture dislocation if untreated.

In addition, with the recent introduction of fixed angle devices, many radius fractures that would have required dorsal support can now also be managed with volar fixation.

Exposing the Radius – Lateral Column

Make a straight longitudinal incision directly over the Flexor Carpi Radialis (FCR). If the incision is to be extended beyond the wrist crease, then it is directed at 45 degrees radially (Fig. 3). Mobilize the FCR ulnarly and incise the floor of the FCR tendon sheath. The musculo-tendinous portion of Flexor Pollicis Longus (FPL) will be encountered and is retracted ulnarly exposing the Pronator Quadratus (PQ). Detach the fibers of the pronator quadratus from the lateral (radial) most aspect of the radius and elevate the PQ from the bony surface and retract it ulnarly. The fibers of the PQ are intimately associated with the insertion of the Brachioradialis (BR), and as such the PQ can be elevated with a slip of BR to assist with later re-approximation. In addition, if the fracture involves the area of the BR insertion then that insertion is divided, alleviating one of the major deforming forces to fracture reduction.

Exposing the Radius – Medial Column

An extended carpal tunnel exposure is preferred. A standard curvilinear, proximal palmar incision is carried proximally onto the volar aspect of the forearm. Care is taken not to cross the wrist flexion creases at a right angle, but to traverse these creases at approximately a 45° inclination. As the incision is carried more proximally, it runs in a line parallel to and about 1cm ulnarward of the palmaris longus tendon. The antebrachial fascia and contiguous transverse carpal ligament are now divided. The interval between the flexor sublimis and flexor profundus bundle and the ulnar neurovascular structures with the flexor carpi ulnaris tendon is developed. Deep dissection along this plane allows retraction of the FDS/FDP and associated median nerve in a radial direction and the FCU and ulnar nerve in an ulnar direction. The pronator quadratus can now be visualized. Elevation of the PQ in a

radial direction allows for complete exposure of almost the entire distal radius, as far radially as the radial styloid, as well as the entire volar ulnar corner of the lunate facet.

With elevation of the PQ volar lip of the radius, the volar radiocarpal ligaments will be seen distally (Fig. 3). Do not open the volar wrist capsule; this compromises vascularity of the fracture fragments and stability of the radio carpal joint. For direct visualization of the articular surface, perform a dorsal arthrotomy or arthroscopy through a dorsal wrist portal.



Fig. 3

Dorsal Approach

The dorsal approach is generally indicated for extra-articular and intra-articular fractures with dorsal displacement and dorsal metaphyseal comminution as well as fractures of the radial styloid and fractures involving the dorsoulnar aspect of the lunate facet.

Exposing the Radius

For radial styloid fractures, an approach between the second and third dorsal compartments is preferred. The second compartment is easily palpable containing the two radial wrist extensors. A longitudinal incision immediately radialward of the second compartment exposes the radial styloid. Careful attention to the superficial branch of the radial nerve is warranted as it runs over the radial styloid and the second compartment. The radial artery is also at risk as it passes around the styloid into the anatomical snuffbox, especially if the incision is extended distally.

Articular reduction can best be assessed through a partial arthrotomy of the wrist between the second and third compartments and one can also see if the scapholunate ligament has been disrupted when the radial styloid fracture is severely displaced proximally.

Dorsal exposure of the distal radius for metaphyseal and central articular fractures is most readily accomplished by opening the third dorsal compartment. A longitudinal incision beginning in the vicinity of Lister's tubercle and extending distally directly exposes the third compartment. The compartment is sharply incised, taking care to avoid damage to the extensor pollicis longus tendon (EPL). The EPL tendon is mobilized and retracted radially, with subperiosteal dissection of the second compartment radially and the fourth compartment ulnarly, allowing complete exposure of the distal radial and dorsal articular fracture fragments.

Following application of the plate, part of the implant will lie under the fourth compartment and the rest will lie under the third and second compartments. During closure the retinaculum flap is used to cover the plate radially leaving the EPL in a subcutaneous position.

Articular fracture reduction

Using the interdigitation of metaphyseal fracture fragments and image intensification, the articular fracture is reduced and held in place with provisional K-wire fixation. K-wires that are essential for fracture reduction, but which interfere with placement of the volar plate, can be driven out through the dorsum of the wrist leaving 1-2mm exposed on the volar surface and 4-5mm protruding out the skin. These pins will be removed after the plate is secured.

Plate Positioning

Use the appropriate Metaphyseal Jig to thread the appropriate number of Standard Cannulas into the holes in the metaphyseal portion of the plate prior to placing the plate on the bone (Fig. 4).

Remove the Metaphyseal Jig.

Apply the appropriate length Periarticular Distal Radial Locking Plate to the bone and position it in the desired location using anatomic landmarks and fluoroscopic images (Fig. 5).

Distal fracture fragment stabilization is optimized when the subchondral support lies immediately below the articular surface. In the distal radius, the articular surface is concave in more than one plane, making accurate tangential radiographic assessment difficult. **Inaccurate reduction and stabilization of the joint may cause the metaphyseal screws to penetrate the articular surface.**



Fig. 4

NOTE: The Metaphyseal Jig and Standard Cannulas **MUST** be used to ensure that the screws align properly with the threaded plate holes. Failure to use the Metaphyseal Jig and Standard Cannulas may result in cross-threading or improper seating of the screws.

A forty-five degree (45°) pronated oblique view* will effectively display the relationship between the dense subchondral bone and the support hardware to verify implant placement.

To obtain the pronated oblique view, the forearm is pronated 45° from either a PA or anteroposterior projection with the horizontal x-ray beam centered on the wrist or a vertically oriented beam and the wrist supinated 45° from full pronation.

Because the radial shaft may not be aligned with the distal fragment, the plate head should be used to determine the appropriate placement of the plate. The plate head should conform to the shape of the distal radius.

Once distal fixation is achieved, the plate/distal radius construct will be reduced to the radial shaft.



Fig. 5

WARNING: Do not contour or bend the plate at or near a threaded hole, as doing so may deform the threaded hole and cause incompatibility with the Locking Screw.

* D.W. Smith and M.H. Henry, *J Hand Surg* 2004; 29A:703-706.

While holding the plate securely in place, reduce the distal fragments by inserting 1.6mm Kirschner wires through the appropriate 1.8mm holes in the head of the plate (Fig. 6). The holes are designed to allow the wires to be angled. After inserting the first wire, check the position of the plate and, if necessary, adjust the position of the plate as necessary. Then insert additional Kirschner wires in the other 1.8mm holes in the head of the plate. The wires will help reduce the articular segment and stabilize the plate while drilling the screw holes.

Additional 1.25mm or 1.6mm Kirschner wires or screws may be placed outside the plate to help reduce or hold fracture fragments in place.

Alternatively, loosely insert a 2.4mm conical screw or a 2.7mm cortical screw into the first slot in the plate shaft. Adjust the plate position proximally or distally as necessary. When the plate is in the desired location, tighten the screw.

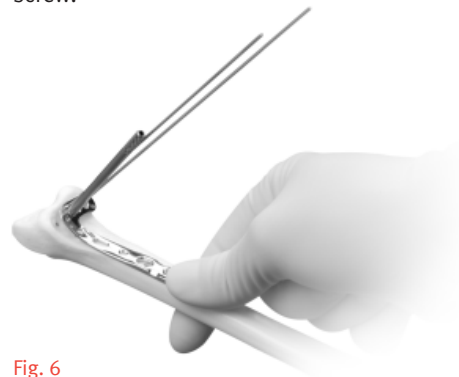


Fig. 6